

## **RAPID, LOW-COST, FULL-WAVEFORM MAPPING AND ANALYSIS WITH ULTRASONIC ARRAYS**

D. Lines<sup>1</sup>, J. Skramstad<sup>2</sup>, and R. Smith<sup>3</sup>

<sup>1</sup> Diagnostic Sonar Ltd, Livingston, West Lothian, UK; <sup>2</sup> NDT Solutions Inc, New Richmond, WI, USA; <sup>3</sup> QinetiQ Ltd, Farnborough, Hampshire, UK

**Abstract:** Many ultrasonic techniques have been proposed for large-area inspection but few can achieve the quality and versatility of information contained in the ultrasonic RF waveform. However inspection speed has always been an issue.

Phased arrays can offer very rapid area coverage rates and the data acquisition and processing technology used for real-time B-scan imaging means that the full-waveform can be acquired without compromising inspection speed. The FlawInspecta system is capable of a pulse rate up to 30kHz, corresponding to a scan rate of 1.8sq.m/minute for 1mm pixel resolution, and so the actual inspection rate is only constrained by the acoustic properties of the material. This scan rate includes simultaneous full waveform capture.

This approach has now been extended, by integration with the ANDSCAN<sup>®</sup> mapping system, so as to provide seamless, full-waveform acquisition over large areas with accurate absolute position of each waveform relative to the structure. The availability of this 3D data set allows a wide range of post-processing options, from multiple gates to spectral analysis, and these post-processing options and many others have been incorporated into a waveform-analysis software plug-in. Full waveform capture allows all of these post-processing options to be done offline so minimizing on-site inspection time.

The paper reports on the improvements to the array and scanning system and outlines how the rapid acquisition of full waveform data can simplify the way that inspections are performed and ensure the future compatibility of the stored data.

**Introduction:** Aircraft include many safety critical components that require non-destructive testing (NDT) at manufacture and throughout the service life. There are many complementary approaches (e.g. visual inspection, radiography, eddy current) and each has its own advantages. However the ability to detect and quantify small mechanical defects at a range of depths within the structure has ensured that ultrasonic inspection techniques have become widely used. Large area inspections are inherently time-consuming and the cost of both this and the associated downtime are considerable limitations. Some novel techniques (e.g. Lamb waves<sup>(1)</sup>) have been developed to scan an area from a single probe placement so as to reduce the time and cost. However the high-resolution requirement precludes the use of these in most aerospace applications and so pulse-echo inspection at each point on the surface of the structure remains the preferred technique.

It is necessary to generate a map of the acoustic measurements at each point on the surface to ensure 100% coverage and to document the inspection<sup>(2)</sup> but inspection time remains a problem. One approach is to speed up the conventional methods by using automated scanners and systems are available that scan either a single transducer in a raster scan or several single-element transducers simultaneously<sup>(3)</sup>. An alternative is to use electronic stepping of the beam along a linear array of transducer elements and then scan this array over the surface<sup>(4-8)</sup>.

These techniques are accelerated versions of conventional inspection of an area where the output is a map of the desired acoustic parameter, such as echo amplitude or time-of flight. However, the reduced inspection time is not the only benefit for the array systems because the very rapid acquisition allows interactive B-scanning that can greatly assist in the detection, localization and characterization of flaws<sup>(8)</sup>.

All the above methods require the equipment to be correctly configured to derive the desired acoustic parameter at acquisition time. This requires a highly trained NDT inspector so that they can not only ensure that the system is optimally configured but also amend or extend the inspection in response to any indications found.

A solution is to acquire and store the full RF waveform. Many configuration parameters (e.g. gate range, delay and mode) can now be adjusted as part of the post-processing review and analysis process. Novel processing algorithms (e.g. spectral analysis <sup>(9)</sup>) can be tried out on archived data sets – a feature that ensures that new inspections remain “future-proof” against algorithm developments. The main disadvantages lie in the rapid acquisition rates needed and the amount of data to be stored. However recent developments in real-time imaging with arrays and with data storage make this approach practicable.

The paper reports on the development of such a system and outlines the changes to NDT inspection procedures that are likely to result from the use of this technique.

**Discussion:** Ultrasonic phased arrays have now been in use for over 3 decades. The terminology has been adopted from phased array radar but this often leads to confusion and so it is helpful to clarify the different configurations in use for NDT.

**Phased array configuration.** Ultrasonic phased arrays were originally developed for medical cardiac imaging where the small array head size and the electronically steered beam were essential for monitoring the rapid movements of the heart through the small access window between the ribs. Rapid improvements in image quality followed by using large aperture arrays, where the scanning is done by electronic stepping of a dynamically focused beam across the width of the array (see Figure 1), and this soon lead to arrays being almost universally adopted for medical applications.

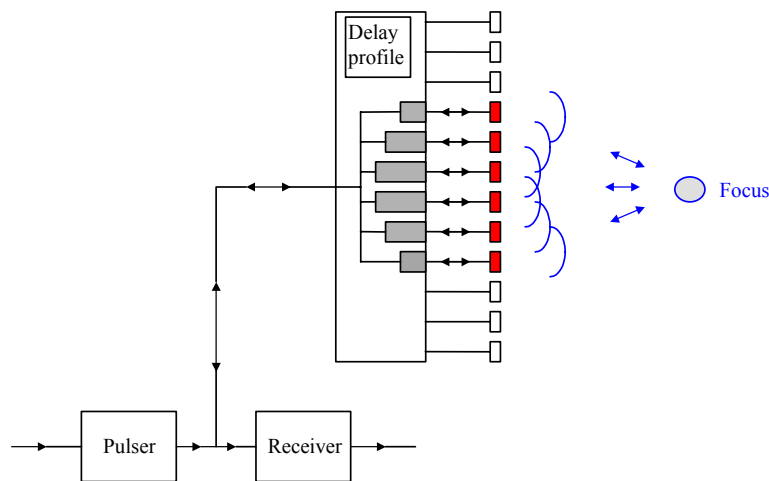


Figure 1. Step-scanned phased array.

The beam is scanned by stepping the active aperture along the length of the array and the focus is altered by adjusting the delays in each channel to compensate for acoustic path differences. It is now over 20 years since Diagnostic Sonar Ltd (DSL) modified one of their medical B-scanners with dynamic focus linear array so as to inspect carbon fiber composite (CFC) airframe structures. There have now been several generations of such equipment.

**Advantages of arrays over automated scanners.** The conventional approach to speeding up area inspections had been to resort to automated inspections <sup>(3)</sup> but arrays offer several advantages:

- The array’s electronic beam-forming ensures that echoes are in focus at all depths so increasing both resolution and sensitivity to small flaws.
- Array fabrication is a high precision process and so there is an inherent accuracy in any measurements made from the B-scan. In addition the overlapping beams ensures 100% coverage irrespective of mechanical backlash tolerances.
- Arrays produce many beams and so the mechanical translation speed is significantly lower than that of a mechanically scanned probe at the same area coverage rate. The coupling

becomes more of a problem at high translation speeds and so the array is at a considerable advantage.

- The propagation time of the ultrasonic pulse is not insignificant at rapid translation rates and the probe is no longer in the same place to receive all the echoes. This not only reduces the sensitivity but also introduces a depth dependent positional error. A raster scan will show this as a backlash that is not easy to compensate since it is depth dependent. The zero-inertia of the array's electronic scan avoids this problem.
- The area coverage rate may ultimately be limited by the combination of material velocity and low attenuation. This requires an additional delay between pulses to avoid confusion with echoes from earlier transmissions. Electronic scanning allows the beams to be fired in any sequence and interlaced fields can be used to operate with minimal delays. Indeed multiple simultaneous beam-forming is used in medical ultrasonic imaging to achieve the maximum scan rates.
- Arrays can be used to produce real-time images and this can greatly assist the operator to detect and characterize flaws when scanning freehand.

**“Smart” arrays.** The medical imaging market has continued to be the driving force behind many of the innovations in ultrasonic phased arrays, such as the adoption of piezo-composite array fabrication. However the wide diversity of NDT inspection requirements requires customized hardware and the cost of this, and of specialized operator training, means that arrays have had far less success in the NDT market.

A modular range of arrays and interface electronics has been developed by DSL to address this combined problem of cost and training. The nature of the application will define the number of elements in the array and whether focusing and steering is required. This in turn allows the selection of the appropriate type and number of standardized electronic modules for interfacing to the array. The use of generic modules ensures that the customization needed for NDT applications can be done at minimum cost. All array controllers feature a common interface design that allows them to operate with a wide variety of equipment - from flaw detectors where the array automatically steps to the next beam on each transmission through to real-time imaging systems that can control all the scan and focus parameters<sup>(7,8)</sup>. The arrays can be small, low-cost and self-multiplexed to be used freehand or in existing scanning systems<sup>(6)</sup> or large, high frequency and wide-band arrays suitable for spectral processing<sup>(4,5,9)</sup>. All are suitable to act as the front-end of a full waveform acquisition system. Coupling is critical and special techniques have been developed to optimize this when scanning at speed<sup>(5)</sup>.

In many cases, especially in aerospace where inspection surfaces often have a high quality finish, the conventional transducer approach of a solid acoustic delay line can be used with arrays, even at speed. However, when the surface is not flat or when the array frequency demands the ultimate in acoustic transmission, it is desirable to use water for coupling and to act as the acoustic delay – in effect mimicking an immersion technique. Bubbler systems offer this capability for automated systems but the extra contact size of an array means that this is often not a practical solution for manual inspection. The approach that has been adopted with some success uses a thin proprietary membrane, acoustically matched to water and hence effectively transparent to the ultrasonic beams, to retain the fluid in front of the array. In the most robust environments, there remains a small gap between membrane and inspection surface that is irrigated so as to accommodate any surface roughness or irregularity such as fasteners. However, the significantly reduced water volume in this region means that it is compatible with manual inspection, even with large arrays. Water recycling or recovery techniques can be used where even the minimal water loss around the skirt is unacceptable. Figure 2 shows the cross sectional geometry and a photograph of a broad band (15MHz center frequency), large aperture (128mm) step-scanned smart- array that is suitable for both imaging and spectroscopy on aerospace lap-joints for corrosion assessment. This implementation was for stand-alone operation and so includes the all the electronics needed for multiplexing and focusing.

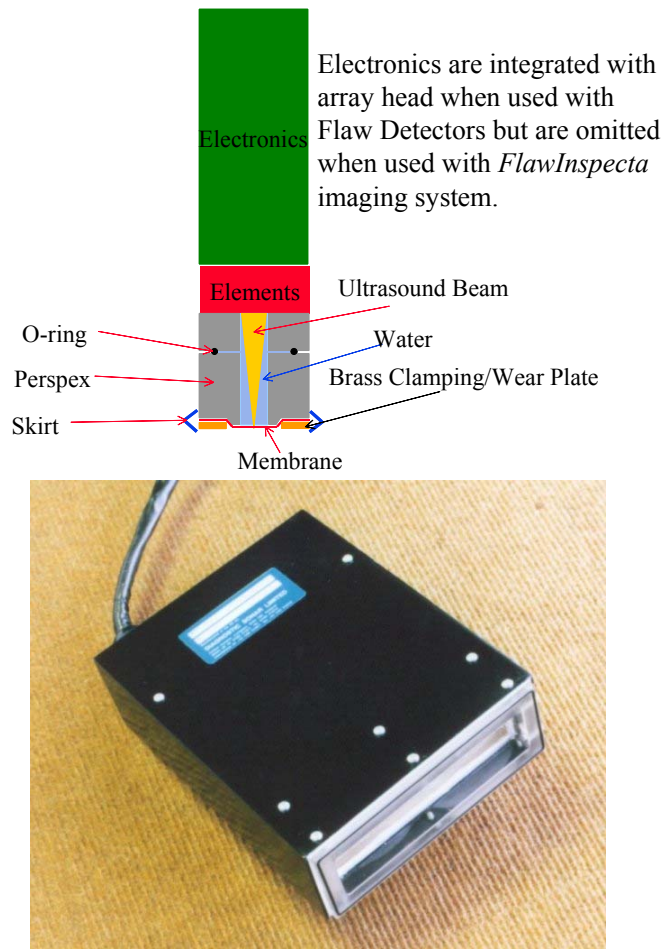


Figure 2. Broadband, high frequency, large aperture “smart” array for corrosion inspection of lap-joints.

**Full waveform acquisition.** In current mapping systems, it is typical that only a single parameter is stored for each pixel on the 2-dimensional surface. The RF A-scan may well have many hundreds of samples and so the full waveform system will need an increase in data acquisition rates and storage of 2 to 3 orders of magnitude. This massive increase requires a different technology but fortunately these requirements are the same as for real-time B-scanning – the only difference being that the data is retained in memory rather than just being directed to the display.

The background to the ultrasonic image acquisition and processing system has been reported elsewhere <sup>(8)</sup> and the frame rate of the current version is constrained only by the acoustic velocity and attenuation of the target material.

**Full waveform analysis.** The availability of the full RF waveform at analysis permits many new operations:

- Spectral filtering (linear and non-linear) is possible both before and after any rectification operation;
- There is no limit on the number of gates and each can be configured to operate on either (or both) signal polarity.
- Gates can be referenced to other gates making it easy to construct interface-following gates and even pre-triggering.

- Arbitrary combinations of results from multiple gates are possible (e.g. the ratio of an echo in one gate divided by the amplitude of the front interface echo in another gate provides an automatic normalization of echoes when the interface is not flat).
- Ultrasonic spectroscopy can be performed over multiple gates so as to implement roughness measurement for corrosion assessment <sup>(9)</sup>.

The Waveform Analysis plug-in to the ANDSCAN<sup>®</sup> mapping system has been developed to perform all of these operations.

The three images in Figure 3 show the Amplitude C-scans for a CFC skin, with a combination of back wall structure and a region of impact damage at the right end, for different gate positions and widths. They illustrate how the data presentation can be optimized as a post-processing function.

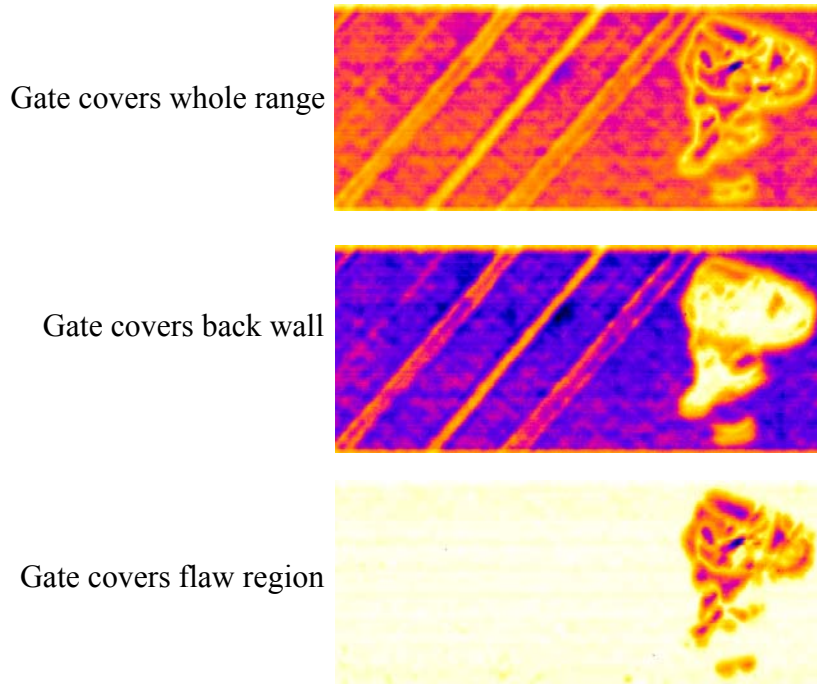


Figure 3. Amplitude C-scans of CFC for different gate positions

Figure 4 shows how the Amplitude and Time of Flight C-scans for a fixed gate can be combined into a composite image for enhanced perception of the structures in a single image. The Amplitude C-scan maps onto intensity while the Time of Flight C-scan maps to hue. The fine detail from the Amplitude C-scan is retained but now the position within the skin of the different features is now readily perceived in a single image.

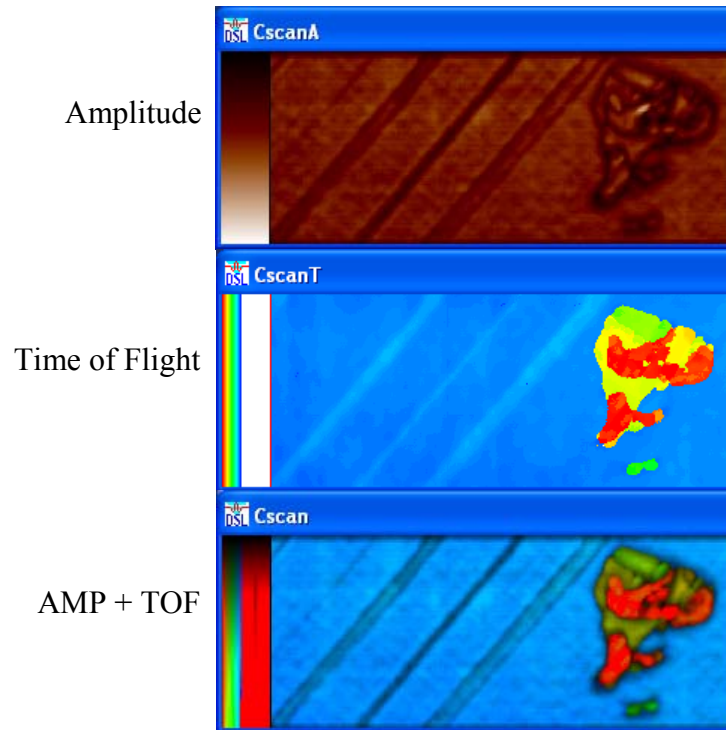


Figure 4. Data fusion of Amplitude and Time of Flight C-scans into composite C-scan

**Implications on inspection procedures.** The ability to manipulate many more parameters at analysis means that the inspection set-up is less critical and could allow the use of a less-qualified inspector. However, it is essential that the data acquired is of high quality and so the dynamic range and the acquisition window must encompass the full range of echoes of interest. In addition, any signal filters must not exclude any frequencies to be analysed later and the digitizer sampling rate and resolution must be adequate to reconstruct the signal accurately.

Quality acoustic coupling must be maintained over the whole area inspected and so some form of monitoring is essential. Experience has shown that a C-scan, derived from gated data that would flag-up a coupling fault, should be used during the scan to monitor the inspection process and to immediate indication of any potential flaws.

The inspection procedure should include documentation of any reference and calibration points (both positional and acoustic). It is also recommended that a quick review should be made of the stored data before leaving the inspection site to ensure that retrieval is possible and indeed standard backup procedures should be followed.

The reduction in inspection time minimizes component downtime and hence cost. Although there can be an increase in analysis time, the separation of the functions means that they can be performed by different personnel with appropriately matched experience. There may be a reduction in the skill level needed for data acquisition operators and it is likely that the most highly skilled personnel will perform the analysis – potentially at a completely different location.

**Modular implementation.** Any practical implementation has to be highly modular so as to address the requirements of a wide range of potential applications. Figure 5a shows a typical system configuration, using the FlawInspecta with R-Theta arm and 0° head, that would be suitable for mapping large areas, such as whole wings, for flaws or corrosion. Figure 5b shows an angled-beam head with self-contained position sensor that can be used for rapid inspection of rows of airframe fasteners for multi-layer cracking. An angled water path, retained by the proprietary acoustically matched membrane, is used to generate the 45° inspection angle. Both

configurations use the same array to ensure that maximum flexibility is achieved at minimum cost.



Figure 5a. ANDSCAN<sup>®</sup> + FlawInspecta system.

Figure 5b. Self-contained angled-beam head

**Conclusions:** It has been shown that there are many advantages in acquiring the full RF waveform for each surface point in an area scanning system. Multiple gate inspections are quicker and all data acquired is available for full offline analysis and so is “future-proof” against algorithm developments. The implications on the inspection procedure, including the possibility of using a less-qualified operator to perform the inspection, have been discussed.

The massive increase in data rates would normally slow down the inspection but DSL’s FlawInspecta technology, developed for real-time B-scanning with ultrasonic arrays has been adapted to maintain rapid inspection speeds at low cost. It has been incorporated into the ANDSCAN<sup>®</sup> mapping system with Waveform Analysis plug-in so that this capability is now commercially available and indeed offers an upgrade path for those with existing mapping systems.

**Acknowledgements:** The authors would like to acknowledge the work of Jamie Bending, David Edgar and Lynn Jones at QinetiQ and also the funding contribution of the UK Ministry of Defence through the Structures Support Group.

© Copyright Diagnostic Sonar and QinetiQ Ltd. and published with the permission of QinetiQ Ltd.

ANDSCAN is a Registered Trademark of QinetiQ Ltd.

**References:**

1. P. Cawley, ‘Practical long range guide wave inspection – applications to pipes and rail’, Proceedings of NDE2002,, Chennai, India, 5-7 December 2002, <http://www.nde2002.org/papers/045P.pdf>.

2. R.A. Smith and L.D. Jones, 'Evaluation and accuracy assessment of ANDSCAN – a non-destructive portable scanner', *INSIGHT - Journal of the British Institute of NDT*, Vol 37, No 4, pp 284-289 and Vol 37, No 5, pp 352-357, 1995.
3. M.K. Reighard, T.W. Van Oordt and N.L. Wood, 'Rapid ultrasonic scanning of aircraft structures', *Materials Evaluation*, Vol 49, No 12, pp 1506-1514, 1991.
4. D.I.A. Lines, K.R. Dickinson, R.A. Smith and S.J. Willsher, 'Optimization of High-Frequency Array Technology for Lap-joint Inspection', *Proceedings of the 3rd Joint DoD/FAA/NASA Conference on Aging Aircraft*, Albuquerque, 1999.
5. R.A. Smith, J.M. Bending, L.D. Jones, T.R.C. Jarman and D.I.A. Lines, 'Rapid Ultrasonic Inspection of Ageing Aircraft', *INSIGHT*, Vol 45, No 3, pp 174-177, 2003.
6. S.J. Willsher and R.A. Smith, 'Multi-element ultrasonic scanning of in-service airframes', *INSIGHT*, Vol 40, No 3, pp 154-159, 1998.
7. D.I.A. Lines, 'Rapid inspection using integrated ultrasonic arrays', *INSIGHT*, Vol 40, No 8, pp 573-577, 1998.
8. D.I.A. Lines, K.R. Dickson, G. Filippi and T. Moir, 'A real-time image acquisition and processing system for ultrasonic arrays in NDT', *Proceedings of NDT'99*, The British Institute of NDT (ISBN 0 903132 27 3), pp.11-17, 1999.
9. R.A. Smith and D.A. Bruce, 'An ultrasonic spectroscopy method for measuring the roughness of hidden corrosion surface', *Proceedings of NDT'98*, The British Institute of NDT (ISBN 0 903132 26 5), pp 167-170, 1998.